

NAVAL HEALTH RESEARCH CENTER

REWARMING METHODOLOGIES IN THE FIELD



*R. S. Pozos
R. L. Hesslink
J. Reading
P. Kincaid
S. Feith*

19950605 037

Report No. 93-4

DTIC QUALITY INSPECTED 3

Approved for public release: distribution unlimited.



NAVAL HEALTH RESEARCH CENTER
P. O. BOX 85122
SAN DIEGO, CALIFORNIA 92186 - 5122

NAVAL MEDICAL RESEARCH AND DEVELOPMENT COMMAND
BETHESDA, MARYLAND

REWARMING METHODOLOGIES IN THE FIELD

R.S. Pozos
R.L. Hesslink
J. Reading
P. Kincaid
S. Feith

Naval Health Research Center
San Diego, California 92186-5122
USA

INTRODUCTION

Hypothermia may occur with prolonged exposure to cold air or water (1,2,3). Recovery from hypothermia involves removing the individual from the cold environment and utilizing a rewarming strategy. Three major rewarming strategies include: 1) passive rewarming, 2) active external heating, and 3) active internal heating. Controversy continues regarding the best rewarming procedure for use in the field.

During passive rewarming, the individual is removed from cold air or water, dried off, placed in a sleeping bag, and allowed to shiver until fully recovered. Provided that the cold stress has been sufficiently removed, it is assumed that the body can spontaneously generate sufficient heat to rewarm itself (2).

Rapid external rewarming is the application of direct heat to the external body surfaces. Rewarming is thus facilitated by heat generated from external sources. Examples of rapid external rewarming include: warm water baths, heat cradles, diathermy, and liquid heated suits (2,3).

Active internal rewarming involves administering heat directly to the "core" of the body, which is usually considered the contents of the trunk beneath the skeletal muscular and adipose shell (2). Examples include: peritoneal dialysis, mediastinal irrigation, extracorporeal circulation, hemodialysis, and intragastric or colonic lavage (2,3). These methods involve surgical procedures and are not practical in a field setting. However, an active internal technique for the field is the breathing of warm, humidified air. Warm moist air is also used in hospitals to help rewarm surgical patients (4,5,6,7,8). The problem is that most of the devices are bulky, heavy, and impractical to use in the field. While investigating a field device used to provide warm humidified air, Sterba (9) had a problem with excessive inspiration temperature.

One study (9) concluded that only passive heating should be done in the field, while others (8,10,11,12,13,14,15) contend that active external, or active internal (5,6,7,8,16,17,18) strategies should be employed. One problem with active external or internal rewarming is that shivering may be decreased, resulting in slower rewarming (13,19). The purpose of this study was to compare the effectiveness of three field rewarming procedures: 1) United States Marine Corps

(USMC) issue extreme cold-weather sleeping bag, 2) cold-weather sleeping bag with external heat applied using a Heatpac device, and 3) cold-weather sleeping bag while breathing warm, humid air from a Heatpac with Humipac (prototype) attachment.

METHODS

Six male subjects participated in this study. The physical characteristics of the subjects are presented in Table 1.

Medical Screening

Subjects were informed of the nature, purpose, and potential risks of the experimental procedures, and they signed informed consent and privacy act statements. All subjects underwent medical screening, which included a medical history questionnaire, body composition assessment, and clearance to participate by a medical officer. Height and weight were determined by standard methods. Body density was determined using skinfolds from three sites: chest, abdomen, and mid-thigh (20). Body fat was determined from body density using the Siri equation (21).

Measurement Systems

A Polar Vantage XL monitor (Polar USA, Inc., Stamford, CT 06902) was used to determine heart rate. Core temperatures were measured using sterile disposable Sher-I-Temp thermistors. Skin temperatures were measured using silver skin thermocouples. A Grant 1200 series (12-Bit) Squirrel Meter/Logger was used to record core and skin temperatures.

Oxygen uptake ($\dot{V}O_2$) and carbon dioxide production ($\dot{V}CO_2$) were determined using open-circuit spirometry. Expired gas was collected for 1.5 minutes in a Collins 100 liter plastic bag connected to a Hans-Rudolph two-way valve. Expired air was analyzed for O_2 and CO_2 using Amatek S-3A/I oxygen and CD-3A carbon dioxide analyzers (Amatek, Pittsburgh, PA), respectively. Expired gas volume was measured using a gas meter (Rayfield Equipment, Waitsfield, VT). Blood pressure was measured using a digital blood pressure monitor (Carolina Biological Supply Co.).

Experimental Protocol

Each subject reported to the laboratory on three separate days within a one-week period. The influence of circadian rhythms on body temperature was controlled by conducting each test at the same time of day (22). Rewarming methods were

presented to each subject in random order. The three methods included passive heating (shivering in the sleeping bag), active external heating (shivering in the sleeping bag with external heat provided by a Heatpac), and active internal heating (shivering in the sleeping bag with Heatpac plus Humipac attachment). The testing protocol consisted of 15 minutes of rest in air at room temperature (23°C), cold water immersion (12.1°C) for up to 85 minutes, four to eight minutes of transition to the rewarming bag, and rewarming for 120 minutes. Measurements included rectal (T_{re}), esophageal (T_{es}), and mean weighted skin temperatures (T_{msk}) (23), as well as heart rate (HR) and oxygen uptake (VO_2).

Subjects fasted for 10 hours prior to each test. Upon arrival to the laboratory, body weight was recorded. Each subject then inserted a rectal thermistor to a depth of 20 cm. An esophageal probe was inserted to heart level. Skin thermistors were placed on the forehead, right cheek, right biceps, right chest, right front mid-thigh, and right back mid-calf. A heart rate telemetry monitor system was placed around the torso at chest level. During the test, each subject wore a bathing suit/shorts.

Baseline measurements of blood pressure, T_{re} , T_{msk} , skin temperatures, HR, and VO_2 were recorded after 15 minutes of rest at room temperature (23°C) immediately before cold-water immersion. Each subject then lowered himself into the cold water bath (12.1°C \pm 1.3) and sat on a chair with the water level up to the apex of the sternum. Recorded cooling time began once the subject was seated. The subject remained in cold water until either his rectal temperature dropped 1°C from baseline, he requested to get out, or after a total elapsed time of 85 minutes. During immersion, HR, T_{re} , T_{msk} , and skin temperatures were recorded every five minutes. At the end of immersion (before exiting the cold-water bath), VO_2 was determined, and body temperatures were recorded again.

After completion of the cold-water immersion, the subject climbed out of the water tank, dried off, changed into dry shorts, and climbed into the sleeping bag placed on a gurney. Transition time into the bag ranged from four to eight minutes. Skin temperatures, T_{re} , and T_{msk} were recorded at five minute intervals throughout rewarming. VO_2 was determined at 15, 45, 90, and 120 minutes of rewarming.

Rewarming Systems

The rewarming systems included: 1) the sleeping bag (SB), 2) sleeping bag with Heatpac (HP) (Alcatel Innova, Norway), and 3) sleeping bag with Heatpac plus Humipac attachment (HHA) (prototype Alcatel Innova, Norway). The sleeping bag was a USMC extreme cold weather bag II, weighing 4.3 kg and rated for temperatures to -50°F. Insulation consisted of waterfowl

feathers, down, and polyester batting.

The Heatpac (HP) is a portable heater weighing 750 g. It utilizes heat from a slow-burning stick of charcoal, assisted by a battery- (size "D" dry cell, 1.5 V) driven fan. The fan pulls air into the unit and pushes it out via heat tubes or tentacles. A catalytic converter removes carbon monoxide and other gases from the burning charcoal. When in use, four heat tubes or tentacles are attached to the HP. The HP is placed inside the sleeping bag near the feet, with the exhaust vented outside of the bag. Inside the bag, two tentacles are placed along the sides of the body, while the other two tentacles are placed on the inside of each thigh.

The Heatpac with Humipac attachment (HHA) is a prototype device that weighs 2.0 kg. Air flows from the HP through the Humipac attachment to a face mask from which the subject inhales and exhales. The Humipac attachment is a double-tube cylinder (one tube inside the other). The inner chamber is lined with a moisture-absorbent material. A 100 ml plastic reservoir is connected to the inner chamber. The reservoir is filled with water, then "squeezed," pushing water into an inner chamber. The moisture-absorbent material then becomes saturated; absorption capacity is 200 g. During operation, warm air flows through the chamber and becomes saturated with water.

During rewarming with the HHA, a temperature probe was placed directly above the area where the warm, humidified air first exits the HHA. The mean near-inspired air temperature exiting the HHA was 50.9 \pm 3.6°C (Fig. 1). The air then travels through a 10 cm rubber neck, through a two-way valve, and into the face mask. Preliminary studies on the HHA (unpublished data) reflect actual inspired air temperatures 2 to 6°C less than temperature coming directly out of Humipac. For this study, the range of air temperature entering the mouth ranged from 45.4 to 47.9°C.

In this study, the charcoal fuel element was ignited at the start of immersion, allowing the HP and HHA to warm up for at least 40 minutes. In all tests, the HP or HHA was set on its highest temperature setting. The HP produced air temperatures of 64.9 \pm 0.8°C (Fig. 1).

During rewarming, the HHA is placed on the subject's chest. The subject's nose and mouth are covered by a standard oral-nasal mask, and the subject inhales warm, humid air. Exhalation is vented to the atmosphere by a two-way valve attached to the mask. The main body of the HHA generates heat to the chest area. The HHA has a cloth cover over the HP and Humipac. During each test the relative humidity of the air going to the subject from the HHA was checked before and after application, and was constant at 100 percent. All experiments were conducted at an environmental temperature of 23°C.

Statistical Analysis

Data were analyzed using repeated measures multivariate analysis of variance (MANOVA). The alpha level was set at 0.05. The rate of rewarming was calculated using the rewarming slope (regression line) of the three rewarming methods.

RESULTS

Cold-water immersion ranged from 40 to 85 minutes (71.1 ± 15.0 min). During immersion, T_{re} and T_{sk} initially increased above baseline values in all subjects. After 5 to 15 minutes of cold-water immersion, T_{re} and T_{sk} began to decrease. However, at the end of cold-water immersion, T_{re} and T_{sk} remained above baseline values in five and three of 18 tests, respectively. T_{re} decreased 1°C in four tests whereas T_{sk} decreased in one test (Table 2).

Rewarming Responses

All subjects shivered vigorously during the initial stages of rewarming. However, the intensity of shivering decreased with gradual rewarming of the body. Rewarming for 120 minutes with all three methods was associated with significant ($p < 0.01$) and progressive increases in T_{re} , T_{sk} , and T_{mak} . As rewarming progressed, $\dot{V}O_2$ decreased significantly ($p < 0.01$) in all three rewarming treatments, but no difference between treatments occurred (Fig. 2).

Afterdrop in T_{sk} was $0.6 \pm 0.3^\circ\text{C}$ with the HHA, $0.8 \pm 0.5^\circ\text{C}$ with the HP, and $0.8 \pm 0.3^\circ\text{C}$ with the SB. Afterdrop in T_{re} was $0.7 \pm 0.4^\circ\text{C}$ with the SB, $0.7 \pm 0.2^\circ\text{C}$ with the HHA, and $1.1 \pm 0.3^\circ\text{C}$ with the HP (Fig. 3). No significant differences in afterdrop were found among the three rewarming methods in T_{re} or T_{sk} .

Analysis of the interaction effect between rewarming time and rewarming method reveals that rewarming occurred faster with HHA compared to HP ($p < 0.01$) and SB ($p < 0.01$). With the application of the HHA, HP, and SB, T_{sk} rewarmed at $1.4^\circ\text{C}\cdot\text{hr}^{-1}$, $1.2^\circ\text{C}\cdot\text{hr}^{-1}$, $1.1^\circ\text{C}\cdot\text{hr}^{-1}$ respectively (Fig. 4). With the application of the SB, HHA, and HP, T_{re} rewarmed at $2.0^\circ\text{C}\cdot\text{hr}^{-1}$, $1.6^\circ\text{C}\cdot\text{hr}^{-1}$, and $1.2^\circ\text{C}\cdot\text{hr}^{-1}$ respectively (Fig. 5). The application of the SB method rewarmed subjects significantly faster ($p < 0.01$) than HP.

With the application of the HHA, SB, and HP, the condition mean for T_{sk} was $36.4 \pm 0.2^\circ\text{C}$, $36.3 \pm 0.2^\circ\text{C}$, and $36.3 \pm 0.2^\circ\text{C}$, respectively. The T_{sk} with the HHA was higher ($p < 0.02$) than with the HP. The T_{sk} condition mean for HHA was similar to T_{sk} with the SB. With the application of the HHA, SB, and HP, the condition mean for T_{re} was $36.2 \pm 0.4^\circ\text{C}$, $36.1 \pm 0.3^\circ\text{C}$, and $36.0 \pm 0.2^\circ\text{C}$, respectively. The T_{re} with the HHA was higher ($p < 0.02$) than the T_{re} with the HP. The T_{re} condition mean for HHA was similar to T_{re} with the SB.

The rewarming rate for T_{mak} was similar among the three rewarming methods (Fig. 6). However, the condition mean for T_{mak} was $32.0 \pm 1.4^\circ\text{C}$ for HP, $31.6 \pm 0.5^\circ\text{C}$ for HHA, and $30.4 \pm 1.2^\circ\text{C}$ for SB; with the HP greater ($p < 0.01$) than the SB, and the HHA ($p < 0.05$) greater than the SB.

DISCUSSION

This study compared three different strategies applicable to rewarming individuals in the field. Our analysis suggests the HHA is the most effective and safest rewarming method.

Investigators have shown that T_{sk} is the more reliable estimation of core temperature (24,25). When using T_{sk} , the findings suggest that the HHA rewarmed subjects faster and tended to have a lower (although not significant) afterdrop than either the HP or SB. An unknown portion of this afterdrop occurred prior to commencement of the treatments. Using a larger sample size in future studies may show a significant reduction in afterdrop for T_{sk} in these different conditions.

External heating using the HP system significantly increased T_{mak} . However, the external heating appeared to suppress the rise in core temperature as indicated by the changes in T_{re} and T_{sk} . The T_{mak} with HHA was higher than with the SB; with the HHA the core temperatures were higher or similar to the temperatures associated with the SB or HP. The HHA warms the skin surface more than the SB, and raises core temperature more than the HP. When significant differences are computed for T_{sk} , T_{re} , and T_{mak} , the HHA is either similar or faster at rewarming than the SB or HP. In addition, the treatment for T_{sk} , T_{re} , and T_{mak} were similar or higher for the HHA than the SB or HP.

In conclusion, the Heatpac with the Humipac attachment supplying warm, humidified air, may be the preferred rewarming device for use in the field, but further research is necessary.

REFERENCES

1. Keating, W.R. (1969). Survival in cold water. Oxford, England. Blackwell Scientific Publishers.
2. Pozos, R.S. & Born, D.O. (1982). Hypothermia causes, effects, prevention. Piscataway, New Jersey. New Century Publishers, Inc.
3. Pozos, R.S. & Wittmers, L.E. (1983). The Nature and Treatment of Hypothermia. University of Minnesota. Minneapolis, Minnesota.
4. Chamney, A.R. (1969). Humidification requirements and techniques. Anaesthesia, 24, 602-616.

5. Hayward, J.S., & Steinman, A.M. (1975). Accidental hypothermia: An experimental study of inhalation rewarming. Aviation Space and Environmental Medicine, 46(10), 1236-1240.
6. Lloyd, E.L. (1973). Accidental hypothermia treated by central rewarming through the airway. British Journal of Anaesthesia, 45, 41-48.
7. Lloyd, E.L. (1990). Airway warming in the treatment of accidental hypothermia: A review. Journal of Wilderness Medicine, 1, 65-78.
8. Hamlet, M.P. (1976). Resuscitation of accidental hypothermia victims. United States Research Institute of Environmental Medicine. Report No. T 42/76.
9. Sterba, J.A. (1991). Efficacy and safety of pre-hospital rewarming techniques to treat accidental hypothermia. Annals of Emergency Medicine, 20(8), 896-890.
10. Daanen, H.A.M., & Van de Linde, F.J.G. (1992). Comparison of four noninvasive rewarming methods for mild hypothermia. Aviation Space and Environmental Medicine, 63, 1070-6.
11. Hesslink, R.L. Jr., Pepper, S., Olsen, R.G., Lewis, S.B., & Homer, L.D. (1989). Radio frequency (13.56 Mhz) energy enhances recovery from mild hypothermia. Journal of Applied Physiology, 67(3), 1208-1212.
12. Marcus, P. (1978). Laboratory comparison of techniques for rewarming hypothermia casualties. Aviation Space Environmental Medicine, 49(5), 692-697.
13. Olsen, R.G. (1988). Reduced temperature afterdrop in Rhesus monkeys with radio frequency rewarming. Aviation Space and Environmental Medicine, 59, 78-80.
14. Romet, T.T., & Hoskin, R.W. (1988). Temperature and metabolic responses to inhalation and bath rewarming protocols. Aviation Space and Environmental Medicine, 59, 630-634.
15. White, J.D., Butterfield, A.B., Greer, K.A., Schoem, S., Johnson, C., & Holloway, R.R. (1984). Comparison of rewarming by radio wave regional hyperthermia and warm humidified inhalation. Aviation Space and Environmental Medicine, 55, 1103-1106.
16. Lloyd, E.L. (1974). Accidental hypothermia: Central rewarming in the field. British Medical Journal, 4, 717.
17. Lloyd, E.L., & Croxton, D. (1981). Equipment for the provision of airway warming (insulation) in the treatment of accidental hypothermia in patients. Resuscitation, 9, 61-65.
18. Shanks, C.A., & Marsh, H.M. (1973). Simple core rewarming in accidental hypothermia. British Journal of Anaesthesia, 45, 522-525.
19. Harnett, R.M., Pruitt, J.R., & Sias, F.R. (1983). A review of the literature concerning resuscitation from hypothermia: Part I - The problem and general approaches. Aviation Space and Environmental Medicine, 54(5), 425-434.
20. Pollock, M.L., Schmidt, D.H., & Jackson, S. (1980). Measurement of cardiorespiratory fitness and body composition in the clinical setting. Comprehensive Therapy, 6(9), 12-27.
21. Siri, W.E. (1961). Techniques for Measuring Body Composition. In: J. Brozek and A. Henschel (Eds). National Academy of Science, pp. 223-244. Washington D.C.
22. Hagan, R.D., & Horvath, S.M. (1978). Effect of diurnal rhythm of body temperature on muscular work. Journal of Thermal Biology, 3, 235-239.
23. Ramanathan, N.L. (1964). A new weighting system for mean surface temperature of the human body. Journal of Applied Physiology, 19(3), 531-533.
24. Brengelmann, G.L. (1987). Dilemma of Body Temperature Measurement. In: K. Shiraka & M. K. Yousef (Eds.), Man in Stressful Environments: Thermal and Work Physiology. pp. 5-21. Springfield, Illinois. Charles C. Thomas.
25. Hayward, J.S., Eckerson, J.D., & Kemna, D. (1984). Thermal and cardiovascular changes during three methods of resuscitation from mild hypothermia. Resuscitation, 11, 21-33.

Table 1. Physical characteristics of the subjects


Subject	Age (yrs)	Height (cm)	Weight (kg)	Body Fat (%)
1	34	186.1	93.6	17.6
2	35	170.2	70.6	9.0
3	25	184.2	89.8	23.1
4	35	181.6	89.6	16.9
5	29	168.9	80.6	17.9
6	29	175.9	106.3	24.4
Mean \pm SD	31 \pm 2	177.8 \pm 3.0	88.4 \pm 4.9	18.1 \pm 2.2

Table 2. Baseline to end of immersion changes (n=18 tests)

Measurement	Baseline	End of Immersion	Difference
T_{re} ($^{\circ}$ C)	37.0 \pm 0.2	36.6 \pm 0.6	0.4 \pm 0.5
T_{es} ($^{\circ}$ C)	36.8 \pm 0.2	36.5 \pm 0.6	0.3 \pm 0.5
T_{msk} ($^{\circ}$ C)	29.1 \pm 1.1	18.8 \pm 1.3	10.4 \pm 2.9*
$\dot{V}O_2$ (l \cdot min $^{-1}$)	0.35 \pm 0.05	1.08 \pm 0.29	0.73 \pm 0.28*
HR (bpm)	68 \pm 10	77 \pm 8	9 \pm 14


* $p < 0.05$

Fig. 1 Heatpac Tentacle and Humipac Near-inspired Air Temperature

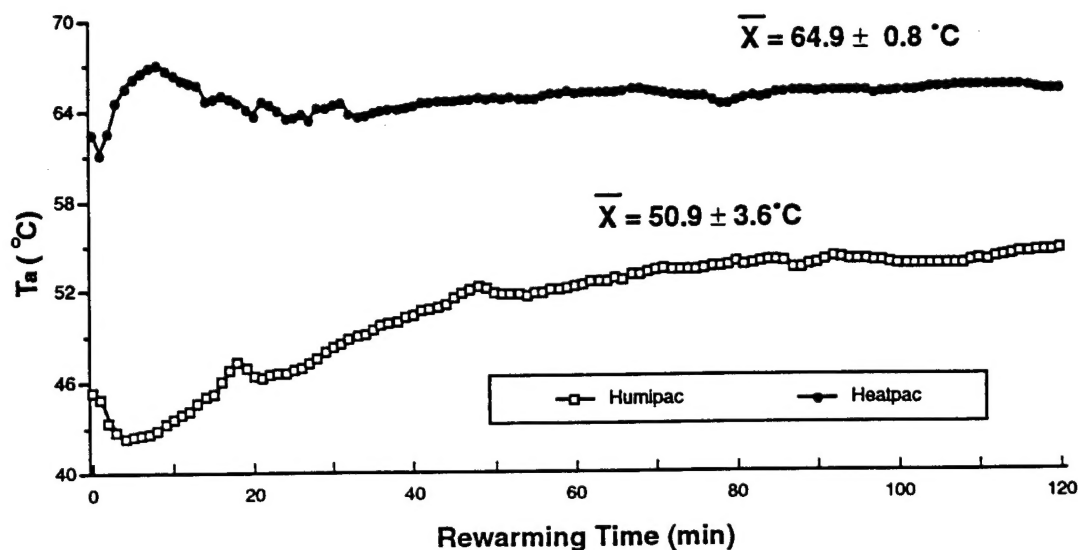

Note: Actual inspired air temperature is predicted to be 45.4-47.9°C (authors unpublished data).

Fig. 2 Oxygen Uptake During Three Rewarming Protocols

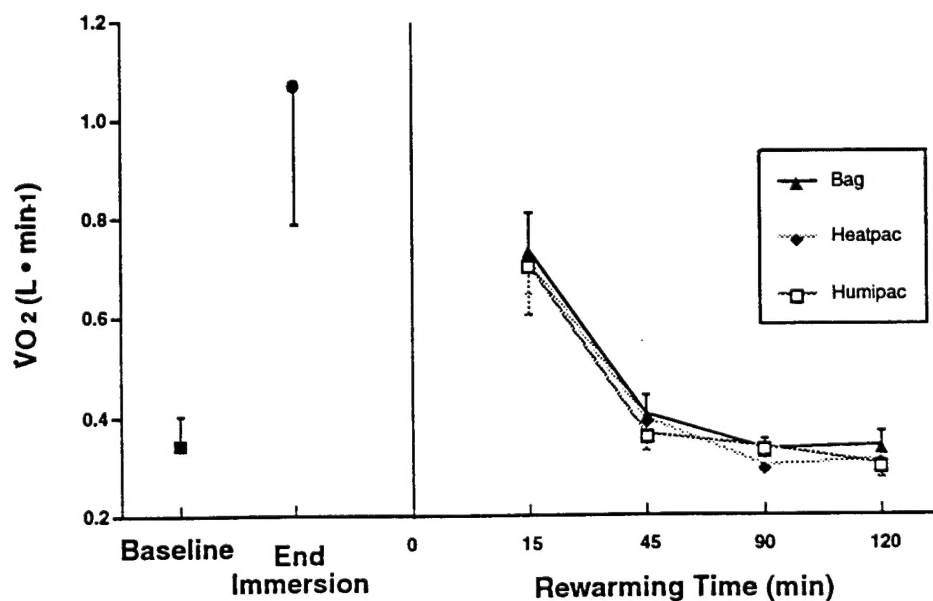

Note: Baseline and end immersion scores for HHA (n=6), SB (n=6), and HP (n=6) were similar. Baseline and end immersion scores were determined using n=18.

Fig. 3 Esophageal and Rectal Temperature Afterdrop



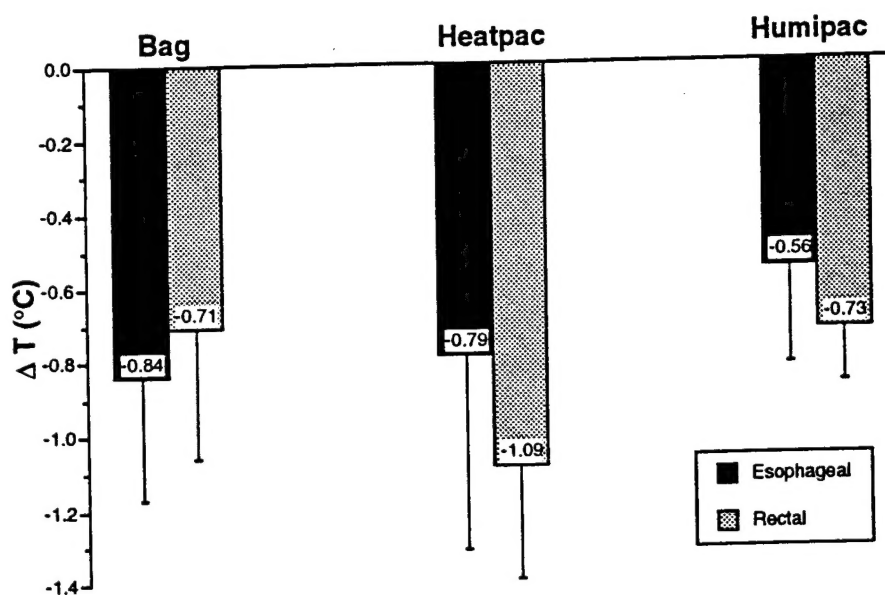


Fig. 4 Mean Esophageal Temperature During Rewarming

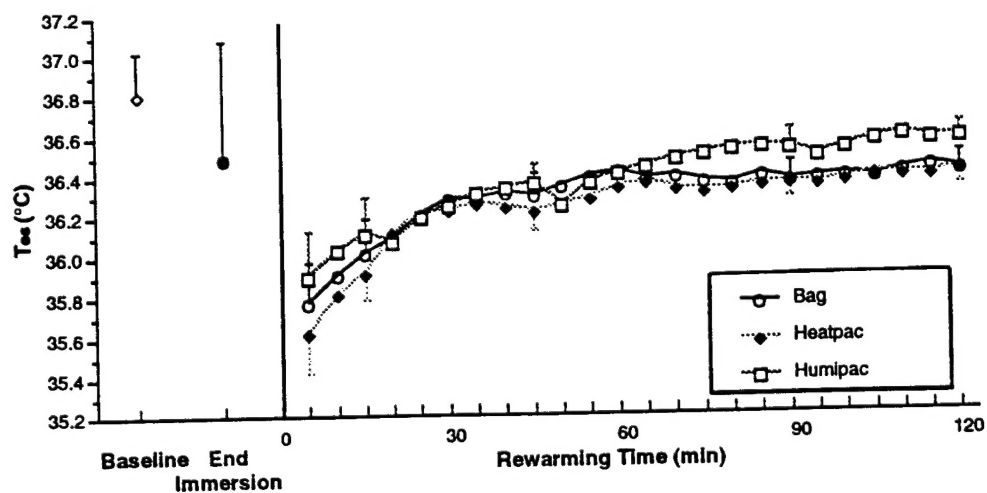


Note: Baseline and end immersion scores for HHA (n=6), SB (n=6), and HP (n=6) were similar. Baseline and end immersion scores were determined using n=18.

Fig. 5 Mean Rectal Temperature During Rewarming

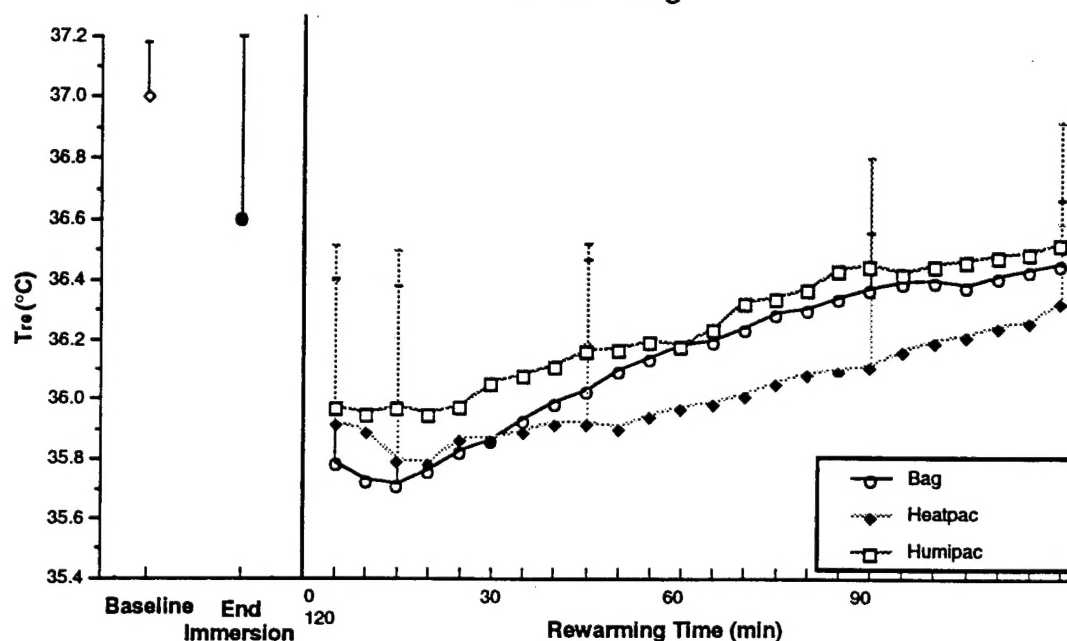

Note: Baseline and end immersion scores for HHA ($n=6$), SB ($n=6$), and HP ($n=6$) were similar. Baseline and end immersion scores were determined using $n=18$.

Fig. 6 Mean Skin Temperature During Rewarming

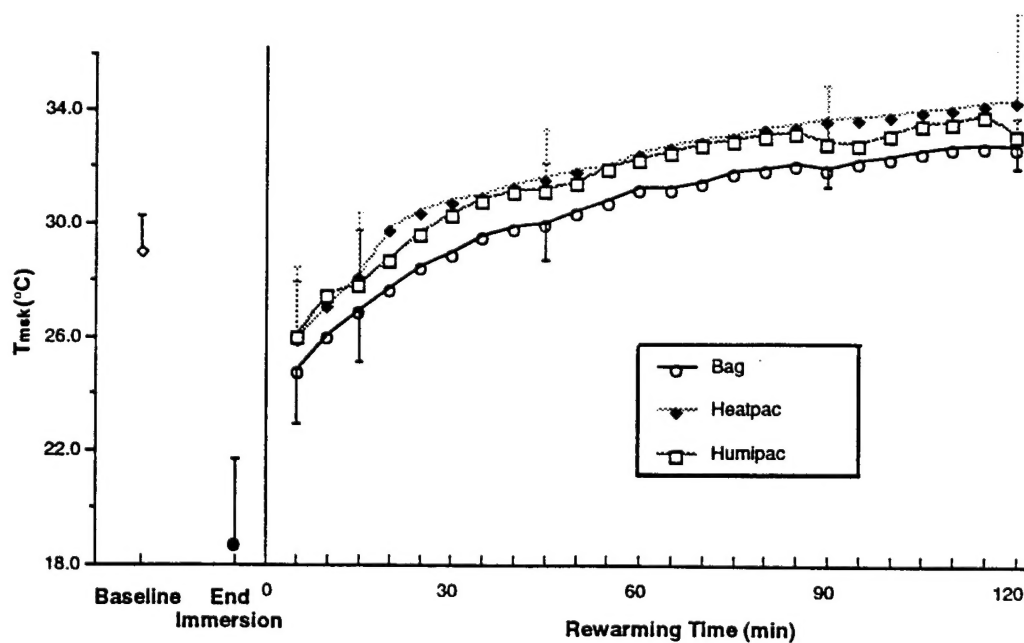

Note: Baseline and end immersion scores for HHA ($n=6$), SB ($n=6$), and HP ($n=6$) were similar. Baseline and end immersion scores were determined using $n=18$.

REPORT DOCUMENTATION PAGE			Form Approved OMB No. 0704-0188	
Public reporting burden for this collection of information is estimated to average 1 hour per response, including the time for reviewing instructions, searching existing data sources, gathering and maintaining the data needed, and completing and reviewing the collection of information. Send comments regarding this burden estimate or any other aspect of this collection of information, including suggestions for reducing this burden, to Washington Headquarters Services, Directorate for Information Operations and Reports, 1215 Jefferson Davis Highway, Suite 1204, Arlington, VA 22202-4302, and to the Office of Management and Budget, Paperwork Reduction Project (0704-0188), Washington, DC 20503.				
1. AGENCY USE ONLY (Leave blank)		2. REPORT DATE Nov 17, 1993		3. REPORT TYPE AND DATE COVERED Technical Report
4. TITLE AND SUBTITLE Rewarming Methodologies in the Field			5. FUNDING NUMBERS Program Element: 63706N Work Unit Number: M0096.002-6203	
6. AUTHOR(S) S. Feith, R. Hesslink, J. Reading, P. Kincaid, R. Pozos				
7. PERFORMING ORGANIZATION NAME(S) AND ADDRESS(ES) Naval Health Research Center P. O. Box 85122 San Diego, CA 92186-5122			8. PERFORMING ORGANIZATION Report No. 93-4	
9. SPONSORING/MONITORING AGENCY NAME(S) AND ADDRESS(ES) Naval Medical Research and Development Command National Naval Medical Center Building 1, Tower 2 Bethesda, MD 20889-5044			10. SPONSORING/MONITORING AGENCY REPORT NUMBER	
11. SUPPLEMENTARY NOTES				
12a. DISTRIBUTION/AVAILABILITY STATEMENT Approved for public release; distribution is unlimited.			12b. DISTRIBUTION CODE	
13. ABSTRACT (Maximum 200 words) The Heatpac is currently used by the U.S. Marine Corps to warm cold-stressed infantry personnel in the field. Recently, this system has been modified so a small wetting chamber called Humipac can be attached to the Heatpac so personnel can breathe warm humidified air. The air is saturated to 95-99% humidity with a temperature range of 45.3 to 49.4°C. In a series of experiments using a USMC issue sleeping bag, we compared the effectiveness of the Heatpac vs. combined Heatpac/Humipac vs. rewarming by shivering. Subjects wearing only swimming trunks were placed in 12.8°C water for 1 hr. At the end of that period, any of the three interventions were randomly assigned. In all conditions, the subject was placed in a sleeping bag. HR, T _{re} and T _{es} temperatures, and metabolic rates were monitored during the cooling phase and for 120 min during the rewarming phase. Breathing the warm humidified air did not significantly alter the rate of body rewarming. In some cases, normal shivering induced as large an increase in core temperature as did the active interventions. Additional studies are underway to investigate the relative role that these various rewarming systems have on thermogenesis.				
14. SUBJECT TERMS Rewarming, hypothermia			15. NUMBER OF PAGES 8	
			16. PRICE CODE	
17. SECURITY CLASSIFICATION OF REPORT Unclassified	18. SECURITY CLASSIFICATION OF THIS PAGE Unclassified	19. SECURITY CLASSIFICATION OF ABSTRACT Unclassified	20. LIMITATION OF ABSTRACT Unlimited	